Experiment CM-5: Carbon Dioxide Fixation in Intact Cells

Equipment Required

PC or Mac computer

IXTA, USB cable, power supply

ISE-730 Dissolved oxygen electrode

RPC-100 respiration/photosynthesis chamber

Magnetic stir motor, stir bar, and motor controller

High intensity light source with full intensity control (The Dyna Lume Sun-Lite I is excellent)

Light meter

Vortex mixer

10µl micropipette with gel-loading tips.

Squirt bottle filled with deionized water

Pasteur pipet with plastic tip

The following information is in the Appendix:

- Algal cells in suspension
- HCO_3^- solution
- MA (methylamine) uncoupler solution
- IAA (iodoacetamide) solution
- DCMU (3-(3,4-dichlorophenyl)-1,1-dimethylurea) solution
- Thylakoid suspension
- Thylakoid reaction media
- Concentrated O_2 depletion solution

Warning: The dissolved oxygen electrode has been prepared by the laboratory staff. When you receive your electrode: 1) Handle it carefully. The tip of the electrode is covered by a delicate Teflon(tm) membrane which can tear easily. 2) Do not tighten or loosen the plastic housing holding the Teflon(tm) membrane. Tightening the housing will stretch or tear the membrane; loosening the housing will cause the electrolyte to leak out of the electrode and affect its responsiveness.

Dissolved Oxygen Electrode Setup

1. Locate the dissolved oxygen electrode and plug it into channel A5 on the front of the TA.

Iworx Sample Lab

2. Place the small magnetic stir bar in the bottom of the chamber. Fill the chamber with room temperature deionized water.
3. Install the oxygen electrode into its port on the polarograph chamber.
4. Position the chamber over the center of the magnetic stirrer. Turn on the stirrer, starting at a slow speed. Reposition the chamber over the stirrer so that the stir bar is centered in the chamber. Turn up the speed of the stirrer to the maximum rate that allows the stir bar to rotate evenly.

Figure CM-5-S1: The DO2 attached to the IXTA.

Note: *If the solution in the chamber is stirred, changes in oxygen concentration reach the electrode instantaneously. If a stirrer is not used, changes in the rate of oxygen production are limited by the rate of diffusion.*

iWorx Lab

Figure CM-5-S2:The oxygen polarograph used to record photosynthetic electron transport. Black tape should cover the side of the polarograph block facing the light source, except on the area directly on the front of the chamber. The light is focused on this open area so that the circle of light is only large enough to cover the chamber.

Calibration of Dissolved Oxygen Electrode

Aim: To calibrate the dissolved oxygen electrode.

The standard used for calibrating the dissolved oxygen electrode is the known concentration of oxygen in air-saturated deionized water. The amount of oxygen that is dissolved in water is known as its solubility (S) and it is dependent upon the temperature, oxygen pressure in the air, and the concentrations of dissolved solutes in the water. Solubility (S) can be determined by using the following equation:

$$S = (\alpha/22.414)\ ((P-p)/P)\ (r\%/100).$$

IWorx Sy

In the equation, α is the absorption coefficient of O_2 at the temperature, p is the vapor pressure of water at the temperature, P is the barometric pressure, and r% is the percent oxygen in the air. For example, at 26°C and 760mmHg and a concentration of oxygen in air of 21%, S equals:

$$(0.02783/22.414\text{L/mole})(734.91\text{mmHg}/760\text{mmHg})(0.21) = 252\mu\text{MO}_2$$

Procedure

1. Fill the RPC-100 respiration chamber with fresh deionized water.
    - Turn off the stirrer if it is on.
    - Remove the dissolved oxygen electrode from the RPC-100 respiration chamber.
    - Remove the water from the chamber using a plastic-tipped Pasteur pipet fitted with a bulb.
    - Fill the chamber with fresh room temperature deionized water.
    - Replace the DO2 electrode in its port on the chamber. Make sure there is enough water in the chamber to submerge the tip of the oxygen electrode.
    - Turn on the stirrer and adjust the its speed so the stir bar is rotating quickly and evenly.
2. Type **Saturation-DI Water** in the Mark box.
3. Click Record on the Main window. The recording will eventually reach a stable level near the top of the recording channel. Click the mark button to mark the recording when the output of the electrode is constant. At this point in the recording, the output of the oxygen electrode is equal to the saturation concentration of oxygen in deionized water at room temperature. Click Stop to halt the recording.
4. Follow the procedure described in Step 1 to replace the deionized water in the RPC-100 chamber with zero-percent oxygen calibration solution at room temperature. Make sure there is enough solution in the chamber to submerge the tip of the oxygen electrode.
5. Type **No Oxygen** in the Mark box.
6. Click Record on the Main window. The recording will eventually reach a stable level near the bottom of the recording channel. Click the mark button to mark the recording when the output of the electrode is constant. At this point, the output of the oxygen electrode is equal to no oxygen being dissolved in deionized water at room temperature. Click Stop to halt the recording.
7. Select Save As in the File menu, type a name for the file. Click on the Save button to save the data file.
8. Prepare the chamber for Exercise 1:
    - Turn off the stirrer, and then remove the electrode from the chamber.
    - Hold the electrode over the beaker used for collecting waste liquid, and rinse the electrode with deionized water from a wash bottle. Blot any drops of rinse water from the electrode. Place the electrode in a beaker of deionized water.

IworX Sample Lab

- Remove the oxygen-depleted water from the chamber with a plastic-tipped Pasteur pipet. Rinse the chamber ten times with deionized water.
- Fill the chamber with deionized water. Replace the electrode in the chamber.

Units Conversion

1. Measure the temperature (in ^{o}C) in the lab room. Assume the barometric pressure in the lab room is one atmosphere (760mmHg) and the concentration of oxygen in the air is 21%. From Table 1 find the dissolved oxygen concentration ([O_2]) in deionized water at room temperature.

   This concentration will be used in Step 6 to calibrate the dissolved oxygen electrode.
2. Scroll to the beginning of the calibration data for the dissolved oxygen electrode.
3. Use the Display Time icons on the LabScribe toolbar to adjust the Display Time of the Main window to show the data collected at both the 100% and 0% saturation levels of oxygen in water on the Main window at the same time. The required data can also be selected by:
   - Placing the cursors on either side of data required.
   - Clicking the Zoom between Cursors button on the LabScribe toolbar to expand the segment with both the 100% and 0% saturation levels of oxygen in water to the width of the Main window.

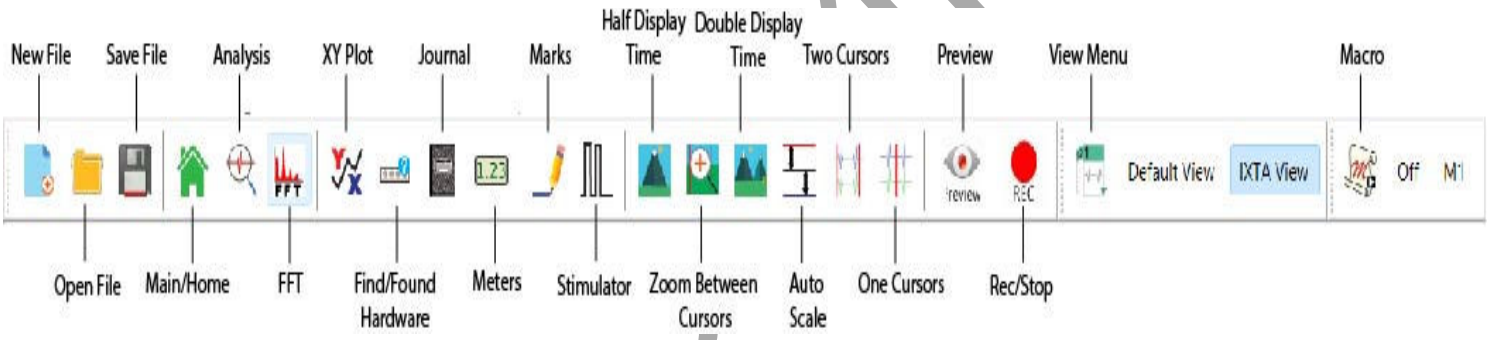

Figure CM-5-S5: The LabScribe toolbar.

4. Click the Double Cursor icon so that two cursors appear on the Main window. Place one cursor on the flat section of data collected when the saturation of dissolved oxygen in water was 100% and the second cursor on the flat section of data collected when the saturation of dissolved oxygen in water was 0%.
5. To convert the output of the dissolved oxygen electrode from a voltage to the molarity of dissolved oxygen in a sample:
   - Click on V2-V1 to the right of the Oxygen channel..
   - Select Simple.

iWorx - Apple Lab

Table CM-5-S1: Concentration of Oxygen [O2] in Air-Saturated Deionized Water at 1 Atmosphere.

Temp (^oC)	O_2 Abs Coeff (a)	H_2O Vapor Press (p in mmHg)	[O2] (µM)
20	.03102	17.54	284
21	.03044	18.65	278
22	.02988	19.83	273
23	.02934	21.07	267
24	.02881	22.38	262
25	.02831	23.76	257
26	.02783	25.09	252
27	.02736	26.74	247
28	.02691	28.35	243
29	.02649	30.04	238
30	.02608	31.82	234

6. The Simple Units Calibration window will appear. On this window:
    - Select 2 point calibration from the pull-down menu in the upper-left corner of the window.
    - Put a check mark in the box next to Apply units to all blocks.
    - Notice that the voltages from the positions of the cursors are automatically entered into the value equations.
    - From Table 1 find the concentration of dissolved oxygen in water at the room temperature that is 100% saturated. Enter this concentration in the corresponding box to the right of the voltage at 100% oxygen saturation. Enter zero in the corresponding box to the right of the voltage for 0% oxygen saturation. Enter the name of the units, µMolar, in box below the concentration. Click on the OK button in the lower right corner of the window to activate the units conversion.

IWorX Sample Lab

Precautions

1. Your use of time in this experiment is critical, since algal cells in suspension are useful for a limited period of time (3 to 4 hours). Complete all the exercises before analyzing the data.
2. The lights in the room will be turned off during the experiment. It is important to gather all the supplies that you will need at your station before the lights are turned off. Some of the items needed close to your work station include: a test tube rack, a micropipette (set to 10µl), disposable gel-loading micropipette tips, a squirt bottle filled with deionized water, a squirt bottle filled with 70% ethanol, Pasteur pipettes with soft plastic tubes on the their tips, a light-tight container for storing the suspension of algal cells, an insulated ice bucket for storing reagents, and reagents.
3. Small amounts of reagents will be dispensed in capped microfuge tubes. Larger amounts should be kept in capped test tubes.
4. Fill your ice bucket halfway. Place a 100ml beaker, for holding your tubes of reagents, in the ice.
5. The capped test tubes with the algal cells will be dispensed when the room lights are turned off. Keep the container with algal cells covered when the cells are inside.

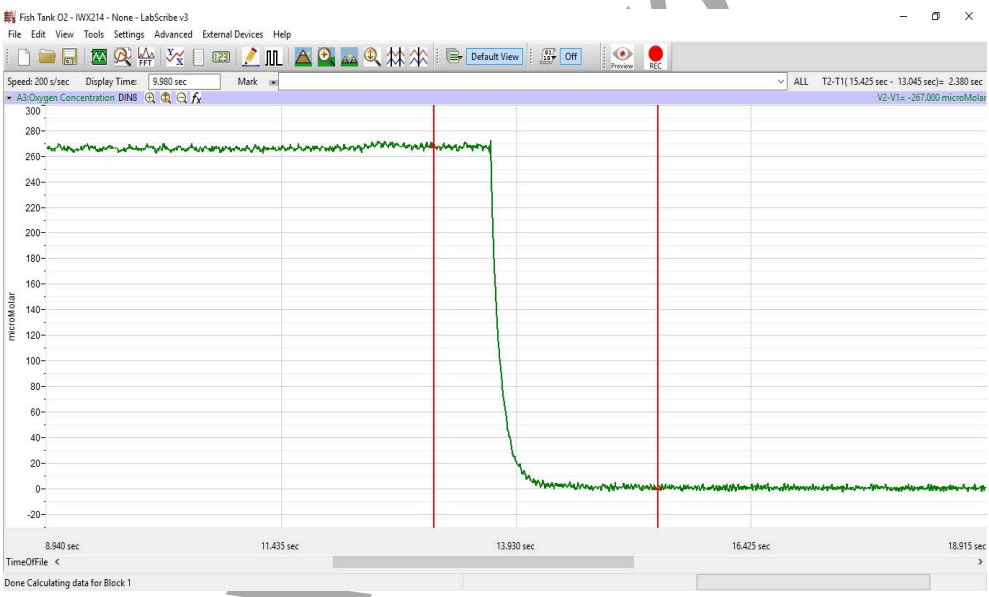

Figure CM-5-S6: Recording of oxygen concentrations in air saturated and oxygen depleted deionized waters used to convert the units of the Y-axis from voltage to O_2 concentration (µMolar).

IWorx Sample Lab

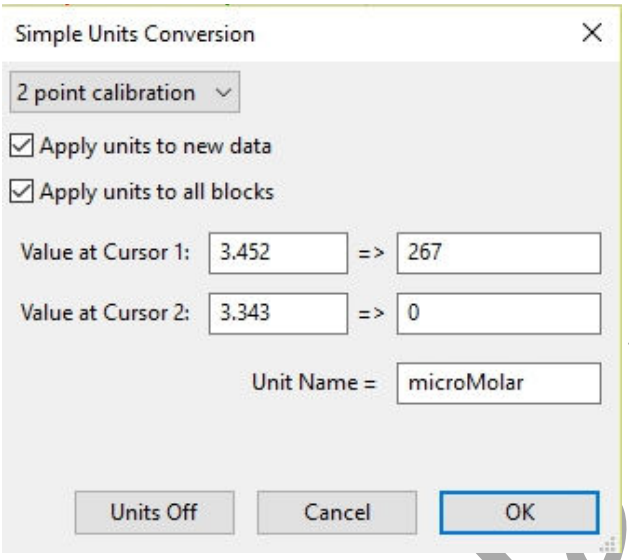

Figure CM-5-S7: The Simple Units Conversion dialogue window with the voltages at the cursors set to equal the dissolved oxygen concentrations used in calibration.

IWorx Sample Lab

Experiment CM-5: Carbon Dioxide Fixation in Intact Cells

Exercise 1: Carbon Dioxide Fixation in the Presence of an Uncoupler

Aim: To determine the rate of oxygen production by algal cells as an indicator of carbon dioxide fixation. This experiment will be performed with and without ATP synthesis being coupled to the electron transport chain.

Approximate Time: 15 minutes

Procedure

1. Turn off the light source used to illuminate the reaction chamber:
    - If the light has a power switch which is separate from the intensity control, use this switch to turn off the light.
    - If the light does not have a separate power switch, plug the light source into a power strip that has a switch. Use the switch on the power strip to turn off the light.
    - While the light is off, set the intensity control of the illuminator to the maximum level (100%).
2. Turn off the stirrer for the chamber. Remove the electrode from the chamber and place it in a beaker of deionized water. Remove the deionized water from the chamber with a plastic-tipped Pasteur pipet. Rinse the chamber two times with deionized water.
3. Make sure no light is reaching the polarograph chamber.
4. Swirl the tube of algae to suspend the cells homogeneously. Fill the chamber with algal cells. Carefully replace the electrode in the chamber and turn on the stirrer.
5. Check the chamber for the presence of bubbles. If bubbles are present, turn off the stirrer, allow the bubble to rise to the top. Remove the electrode and the bubble should burst. Replace the electrode, turn on the stirrer, and check for bubbles, again.
6. Add a 10µl aliquot of HCO_3^- solution to the chamber through the reagent port. Be careful not to add an air bubble to the chamber.

Note: *Put the tip of the micropipette down the reagent port and push its plunger to discharge the 10µl of the HCO_3^- solution into the chamber. Do this carefully so that no bubbles are introduced into the chamber. Remove the micropipette from the chamber before releasing its plunger. If the plunger is released while the tip of the micropipette is still in the chamber, solutions could be siphoned from the chamber.*

7. Type **Algal Cells in Dark** in the Mark box. Position the trace near the bottom of the screen. Click the Record button. Click the mark button to mark the recording. Record the rate of oxygen production of the algal cells in darkness for one minute. Continue recording.
8. Type **Algal Cells in Light at 100%** in the Mark box. Click the mark button as the light is turned on and the algal cell suspension in the chamber is illuminated at the highest intensity.
9. Record oxygen production at this intensity for two minutes. Continue recording.

Work Sample Lab

10. Type **Methylamine Added** in the Mark box. Click the mark button as a 10µl aliquot of methylamine uncoupler solution is added to the chamber through the reagent port. Record the oxygen production of the algal cells exposed to 100% light in the presence of an uncoupler for five minutes.
11. Click Stop to halt the recording.
12. Select Save in the File menu.
13. Remove the electrode from the chamber, and rinse the electrode with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
14. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. Rinse the chamber with deionized water about ten times.

Exercise 2: Carbon Dioxide Fixation in the Presence of a Calvin Cycle Enzyme Inhibitor

Aim: To determine the rate of carbon dioxide fixation (oxygen production) with and without the Calvin Cycle taking place in the algal cells.

Approximate Time: 15 minutes

Procedure

1. Repeat Exercise 1 using Iodoacetamide (IAA) solution in place of Methylamine (MA) solution. Mark the recording at the appropriate times to indicate the absence or presence of light or the presence of the inhibitor.
2. Select Save in the File menu.
3. Remove the electrode from the chamber, and rinse the electrode with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
4. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. Rinse the chamber with deionized water about ten times.

Exercise 3: Carbon Dioxide Fixation in the Presence of an Electron Transport Chain Blocker

Aim: To determine the rate of carbon dioxide fixation (oxygen production) with and without a block across the electron transport chains of the algal cells.

ApproximateTime: 15 minutes

Procedure

1. Repeat Exercise 1 using DCMU (3-(3,4-dichlorophenyl)-1,1-dimethylurea) solution in place of Methylamine (MA) solution. Mark the recording at the appropriate times to indicate the absence or presence of light or the presence of the inhibitor.
2. Select Save in the File menu.

Worx Sample Lab

3. Remove the electrode from the chamber, and rinse the electrode ten times with 70% ethanol and five times with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
4. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. Rinse the chamber ten times with 70% ethanol and five times with deionized water.

Exercise 4: Oxygen Production by Thylakoids in the Presence of an Uncoupler

Aim: To determine the rate of oxygen production by thylakoids, with and without ATP synthesis being coupled to the electron transport chain.

ApproximateTime: 20 minutes

Procedure

1. In this exercise, use thylakoids and thylakoid reaction mixture in place of suspended algal cells.
2. Turn off the stirrer for the chamber. Remove the electrode from the chamber and place it in a beaker of deionized water. Remove the deionized water from the chamber with a plastic-tipped Pasteur pipet. Rinse the chamber two times with deionized water.
3. Fill the chamber with the yellow thylakoid reaction media. Carefully replace the electrode in the chamber and turn on the stirrer.
4. Check the chamber for the presence of bubbles. If bubbles are present, turn off the stirrer, allow the bubble to rise to the top. Remove the electrode and the bubble should burst. Replace the electrode, turn on the stirrer, and check for bubbles, again.
5. Make sure no light is reaching the polarograph chamber.
6. Type **Thylakoids in Dark** in the Mark box. Position the trace near the bottom of the screen. Click the Record button.
7. While in darkness, mix the tube with the thylakoid preparation on the Vortex mixer, so the suspension is even. Use the micropipette to collect a 10 µl aliquot of thylakoids from the tube.
8. Click the mark button as a 10 µl aliquot of thylakoids is added to the chamber through the reagent port. Be careful not to add an air bubble to the chamber. Record the rate of oxygen production of the thylakoids in darkness for one minute. Continue recording.
9. Type **Thylakoids in Light at 100%** in the Mark box. Click the mark button as the light is turned on and the thylakoid suspension in the chamber is illuminated at the highest intensity. Record oxygen production at this intensity for one minute. Continue recording
10. Type **Methylamine Added** in the Mark box. Click the mark button to mark the recording as a 10µl aliquot of methylamine uncoupler solution is added to the chamber through the reagent port. Record the oxygen production of the thylakoids exposed to 100% light in the presence of an uncoupler for one minute. Continue recording.
11. Turn off the light to put the thylakoids in the dark. Record for another minute. Click Stop to halt recording.
12. Select Save in the File menu.

IworX Sample Lab

13. Remove the electrode from the chamber, and rinse the electrode with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
14. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. Rinse the chamber with deionized water about ten times.

Exercise 5: Oxygen Production by Thylakoids in the Presence of a Calvin Cycle Enzyme Inhibitor

Aim: To determine the rate of oxygen production by thylakoids, with and without the Calvin Cycle taking place in the thylakoid suspension.

Approximate Time: 20 minutes

1. Repeat Steps 1 through 11 from Exercise 4. Mark the recording at the appropriate times to indicate the presence of light and the uncoupler, methylamine.
2. After the recording of the effect of methylamine in Step 11 for one minute, type **IAA Added** in the Mark box. Click the mark button as a 10µl aliquot of Iodoacetamide (IAA) inhibitor solution is added to the chamber through the reagent port.
3. Record oxygen production of the thylakoids exposed to 100% light in the presence of iodoacetamide for another minute.
4. Turn off the illuminator to put the thylakoids in the dark. Record for another minute. Click Stop to halt recording.
5. Select Save in the File menu.
6. Remove the electrode from the chamber, and rinse the electrode with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
7. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. Rinse the chamber with deionized water about ten times.

Exercise 6: Oxygen Production by Thylakoids in the Presence of an Electron Transport Chain Blocker

Aim: To determine the rate of oxygen production by thylakoids, with and without a block of the electron transport chain.

Approximate Time: 20 minutes

1. Repeat Steps 1 through 11 from Exercise 4. Mark the recording at the appropriate times to indicate the presence of light and the uncoupler, methylamine.
2. After the recording of the effect of methylamine in Step 11 for one minute, type **DCMU Added** in the Mark box. Click the mark button as a 10µl aliquot of DCMU blocker solution is added to the chamber through the reagent port.
3. Record oxygen production of the thylakoids exposed to 100% light in the presence of DCMU for another minute.

Worx Sample Lab

4. Turn off the illuminator to put the thylakoids in the dark. Record for another minute. Click Stop to halt recording.
5. Select Save in the File menu.
6. Remove the electrode from the chamber, and rinse the electrode ten times with 70% ethanol and five times with deionized water. Make sure there is no water on the electrode before it is replaced in the chamber.
7. Remove the fluid from the chamber using a Pasteur pipet with a plastic tip. rinse the chamber ten times with 70% ethanol and five times with deionized water.
8. At the end of the lab period, rinse the electrode and chamber. Then, fill the chamber with deionized water and place the electrode in the chamber until the next time it is used.

Data Analysis

Rate of Electron Transport

By international consensus, the rate of electron transport in mitochondria is expressed as the rate of oxygen consumption. The units used to express these rates are: moles O_2/hr/mg protein. Oxygen consumption rates are standardized for comparison of experiments performed in different laboratories around the world. The size of the reaction chamber, the amount of mitochondrial protein in the chamber, and the time period for that change in oxygen concentration need to be included in the calculation of the rate.

Early in this experiment, the oxygen probe was calibrated using air-saturated, deionized water at room temperature. Through this calibration, the Y-axis of the recording channel was converted from voltage to oxygen concentration or [Oxygen], which is expressed as μMolarO_2 and abbreviated μMO_2.

Changes in O_2 Concentrations in Exercises 1, 2, & 3.

The rate of change of the oxygen concentration in the polarograph chamber can be measured directly from the recordings by measuring the average slope of the trace (Mean_dv/dt).

Follow these steps to measure the rates of change of the oxygen concentration during these exercises.

1. Scroll through the recording and find the section of data recorded during Exercise 1.
2. Use the Display Time icons to adjust the Display Time of the Main window to show the complete experimental run on the Main window. The complete experimental run can also be selected by:
    - Placing the cursors on either side of the complete run; and
    - Clicking the Zoom between Cursors button on the LabScribe toolbar to expand the complete experimental run to the width of the Main window.
3. Click on the Analysis window icon in the toolbar or select Analysis from the Windows menu to transfer the data displayed in the Main window to the Analysis window.
4. Look at the Function Table that is above the Oxygen Concentration channel displayed in the Analysis window. The functions, V2-V1, T2-T1, and Mean_dv/dt should appear in the table.

iworx Sample Lab

5. Once the cursors are placed in the correct positions for determining the change in the oxygen concentration in the chamber, the values of the parameters in the Function Table can be recorded in the on-line notebook of LabScribe by typing their names and values directly into the Journal.

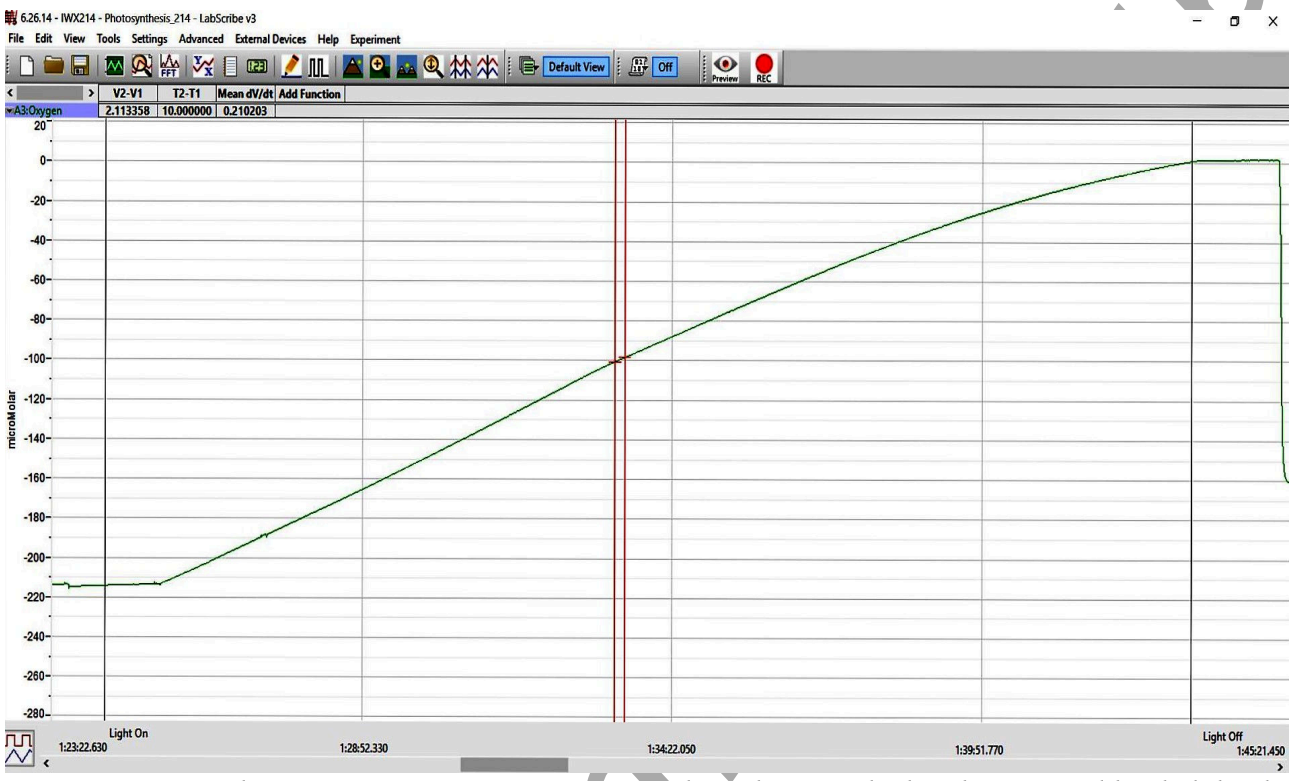

Figure CM-5-L1: Change in oxygen concentration in the polarograph chamber created by thylakoids with whole electron transport chains exposed to 80% light in the presence of an uncoupler. As displayed in the Analysis window, the marks indicate the times when the shutter controlling the light was opened and closed. Cursors are 10 seconds apart. The average rate of change (Mean_dv/dt) in the oxygen concentration over that period is the 0.210203 µMolar O_2/sec.

6. The functions in the channel pull-down menus of the Analysis window can also be used to enter the names and values of the parameters from the recording to the Journal. To use these functions:
    - Place the cursors at the locations used to measure the change in oxygen concentration.
    - Transfer the names of the mathematical functions used to determine the change in oxygen concentration to the Journal using the Add Title to Journal function in the Lung Volumes Channel pull-down menu.
    - Transfer the values for the change in oxygen concentration to the Journal using the Add Ch. Data to Journal function in the Oxygen concentration channel pull-down menu.

IWorx Sa

7. In the Analysis window, use the mouse to click on and drag the cursors to specific points on the recording to measure the following rates:
    - Algal Cells in Dark rate, which is the rate of oxygen production by the algal cells in the absence of light and uncoupler. Set the cursors ten seconds apart on a linear section of the recording of the dark rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
    - Algal Cells in 100% Light rate, which is the rate of oxygen production by the algal cells in the presence of full light. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
    - Algal Cells in 100% Light with Uncoupler rate, which is the rate of oxygen production by the algal cells in the presence of full light and methylamine. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
8. Record the values for these four rates in the Journal using the one of the techniques described in Steps 5 or 6.
9. Use the same technique described in the previous steps to measure and record these rates from:
    - Exercise 2, where IAA is used in place of Methylamine.
    - Exercise 3, where DCMU is used in place of Methylamine.

Changes in O_2 Concentrations in Exercises 4, 5, & 6

In Exercises 4, 5, and 6, the rates of change of the oxygen concentration in the polarograph chamber filled with thylakoids were measured in the absence and presence of light, an uncoupler, and inhibitor, and a blocker. Follow these steps to measure the rates of change in the oxygen concentration in the polarograph chamber during these exercises:

1. Scroll through the recording and find the section of data recorded during the first experimental run in Exercise 4, the oxygen production rates with different light intensities in the absence of an uncoupler.
2. Use the same techniques described for the analysis of Exercises 1, 2, and 3 to display the complete experimental run on the Main window, transfer the data to the Analysis window, selecting the correct positions of the cursors, and transferring the measurements to the Journal.
3. In the Analysis window, use the mouse to click on and drag the cursors to specific points on the recording to measure the following rates:
    - Thylakoids in Dark rate, which is the rate of oxygen production by the thylakoids in the absence of light and uncoupler. Set the cursors ten seconds apart on a linear section of the recording of the dark rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.

IWorx Sample Lab

- Thylakoids in 100% Light rate, which is the rate of oxygen production by the thylakoids in the presence of full light. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
- Thylakoids in 100% Light with Uncoupler rate, which is the rate of oxygen production by the thylakoids in the presence of full light and methylamine. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
- Thylakoids in Dark with Uncoupler rate, which is the rate of oxygen production by the thylakoids in the absence of light and the presence of methylamine. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.

4. For Exercise 5, measure Thylakoids in 100% Light with Uncoupler and inhibitor rate, which is the rate of oxygen production by the thylakoids in the presence of full light, methylamine, and IAA. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
5. For Exercise 6, measure Thylakoids in 100% Light with Uncoupler and Blocker rate, which is the rate of oxygen production by the thylakoids in the presence of full light, methylamine, and DCMU. Set the cursors ten seconds apart on a linear section of the recording of this rate. The value for the Mean_dv/dt is the average rate of change of oxygen concentration (µMolar/sec) over that ten-second period.
6. Make sure all the changes in oxygen concentration are recorded in the Journal.

Standardizing the Rate of Oxygen Production

To standardize the rates of oxygen production (or consumption) according to the adopted convention, the volume of the polarograph chamber, the measured rate of change in oxygen concentration, and the concentration of thylakoids in the chamber must be incorporated into the calculations.

1. Multiply the rate of change in the oxygen concentration by the volume of polarograph chamber. The product of this calculation is the number of moles of oxygen produced in one second. For example, if the change in oxygen concentration is 0.210 microMolar O_2 (µMO_2 or 10^{-6} moles/liter) per second, and the polarograph chamber has a 1.2 milliliter (ml) capacity; then 0.252 nanomoles (nmoles or 10^{-9} moles) of oxygen are produced in one second:

   $(0.210\mu MO_2/sec)(1.2ml) = 0.252$ nmoles O_2 produced in one second.

2. Next, the moles of oxygen produced in one second must be converted to an hourly rate. In our example, if the amount of oxygen produced is 0.252 nmoles O_2 in one second, the hourly production rate is 0.907 micromoles O_2 (µmoles O_2) per hour:

$(0.252 \times 10^{-9}$ molesO_2/sec)(60sec/min)(60min/hr) = 907×10^{-9}moles O_2/hr = 0.907×10^{-6} moles O_2/hr.

Worx Sample Lab

3. Finally, the moles of oxygen produced per hour must be standardized for the amount of thylakoids in the chamber. Clearly, if a chamber contains more thylakoids, the rate of oxygen production will be greater. After the thylakoids are isolated, the laboratory staff determines the concentration of chlorophyll (chl) in the preparation using a spectrophotometer. The concentration of chlorophyll is proportional to the concentration of thylakoids. Then, the lab staff dilutes the preparation with the appropriate volume of buffer to create a stock suspension of thylakoids that has the same approximate concentration of thylakoids in each lab session. In our example, if the concentration of chlorophyll in the stock solution is 2.5 milligrams of chlorophyll per milliliter (mg chl/ml), and 10 µl of thylakoid suspension is added to the polarograph chamber, the amount chlorophyll added to the chamber is 0.025 mg:

(2.5 mg chl/ml)(0.010 ml) = 0.025 mg chlorophyll in the chamber.

To express the rate of oxygen production properly, the hourly rate of oxygen production must be divided by the amount of chlorophyll in the chamber:

$(0.907 \times 10^{-6}$ moles O_2/hr)/(0.025 mg chl) = 22.7×10^{-6} moles O_2/hr/mg chl = 22.7 µmoles O_2/hr/mg chlorophyll.

4. Calculate the rates of oxygen production (or consumption) for each section of each experimental run using the steps presented above.
5. Enter the rates for all the exercises in Table CM-5-L1.

Correction for Non-Zero Dark Rates

1. Sometimes, before the polarograph chamber is illuminated, thylakoids (or cells) will either produce or consume oxygen at a low rate.
    - If the thylakoids are producing oxygen (+ rate) in the dark, then the recorded rate is greater than the actual light-induced rate of oxygen production. The dark rate is adding itself to the actual rate.
    - If the thylakoids are consuming oxygen (- rate) in the dark, then the recorded rate is less than the actual light-induced rate of oxygen production. The dark rate is subtracting itself from the actual rate.
2. When determining the actual rate of oxygen production (or consumption) attributable to light, the non-zero dark rate, whether positive or negative, must be subtracted from the recorded rates in the same experimental run. For example, if thylakoids consumed oxygen at a rate of -9.6 µmoles O_2/hr/mg chl in the dark and produced oxygen at the rate of 22.7 µmoles O_2/hr/mg chl in 100% light, their actual rate of light-induced oxygen production is:

(22.7 µmoles O2/hr/mg chl) - (-9.6µmoles O2/hr/mg chl) = 32.3 µmoles O_2/hr/mg chl

Worx Sample Lab

3. For each experimental run in each exercise, subtract the non-zero dark rate from the recorded light-induced rates to yield the actual light-induced rates. Enter the actual rates in the appropriate columns on Table 1.

Questions

1. Do algal cells consume or produce oxygen when they are in the dark? What happens to the oxygen production rate when the algal cells and reagents in the chamber are exposed to light?
2. What effect does MA (methylamine) have on the oxygen production rates of algal cells?
3. What effect does IAA (iodoacetamide) have on the oxygen production rates of algal cells?
4. What effect does DCMU (3-(3,4-dichlorophenyl)-1,1-dimethylurea) have on the oxygen production rates of algal cells?
5. What effect does MA have on the oxygen production rates of thylakoids?
6. What effect does IAA have on the oxygen production rates of thylakoids?
7. What effect does DCMU have on the oxygen production rates of thylakoids?
8. How do the oxygen production rates of algal cells in the dark, in the light, and in the light with MA compare to the rates from thylakoids under the same conditions?
9. How do the oxygen production rates of algal cells in the dark, in the light, and in the light with IAA compare to the rates from thylakoids under the same conditions? Remember that MA was added to the chamber before IAA was added.
10. How do the oxygen production rates of algal cells in the dark, in the light, and in the light with DCMU compare to the rates from thylakoids under the same conditions? Remember that MA was added to the chamber before DCMU was added.

Reference

Behrens P W, Bingham S E, Hoeksema S D, Cohoon, D L, Cox J C (1989).Studies on the incorporation of CO2 into starch by *Chlorella vulgaris*. Journal Applied Phycology 1: 123-130

Iworx Sample Lab

Table CM-5-L1: Rates of Oxygen Production in Cells and Thylakoids Treated with an Uncoupler, an Enzyme Inhibitor, and an Electron Blocker.

Treatment Exercise	Rate of Oxygen Production (moles O_2/hr/mg chl)								
	No Reagent			Reagent 1			Reagents 1 & 2		
	Dark	Light	Light -Dark	Reagent 1	Light	Light -Dark	Reagent 2	Light	Light-Dark
1-Algae & Uncoupler				MA					
2-Algae & Calvin Cycle Inhibitor				IAA					
3-Algae & Electron Blocker				DCMU					
4-Thylakoids & Uncoupler				MA					
5-Thylakoids & Calvin Cycle Inhibitor				MA			IAA		
6-Thylakoids & Electron Blocker							DCMU		

Worx Sample

Culturing *Chlorella vulgaris*

1. Obtain a culture of *Chlorella vulgaris* (Beijernick's or similar strain) from a biological supply house or a culture collection. Follow the directions included with the culture or use the following steps.
2. Raise the algae in a 1 liter flask filled with 500ml of mineral salts medium.
3. The flask is kept in a lighted environmental room or chamber with an illumination level of 40-90 umol photon/square meter/second at 25°C.
4. Agitation of the culture and the carbon source is provided by bubbling CO_2 rich air (2% v/v CO_2) through the medium.
5. The KNO3 concentration of the culture medium is set to support a cell density of about 1.7 grams/liter. Measure the rate of oxygen production of the stock culture in an oxygen polarograph illuminated with 100% light intensity. If the slope of the oxygen production line is steeper than 45 degrees, dilute the stock culture with deionized water if the cells will be used within a day.

Isolation of Thylakoids

1. Wash 16 fresh spinach leaves (*Spinacia oleracea*) in tap water and pat dry with paper towels.
2. Tear the leaves into small pieces (<4 cm per side) and place the pieces in the chilled (4ºC) jar of a kitchen blender. Pour 200 ml of cold thylakoid isolation buffer, containing 0.4 grams of sodium ascorbate, on top of the leaves.
3. Homogenize the leaves at low speed for 10 seconds until all the large leaf fragments are in a slurry. Then, homogenize the slurry at high speed for 20 seconds.
4. Filter the homogenate through 8 layers of cheese cloth into a 400 ml beaker. Place the collected filtrate in large centrifuge bottles that can be used in high capacity refrigerated centrifuge (IEC CU5000, for example)
5. Spin the filtrate for 2 minutes at 1000 rpm (~1200xG). Collect the supernatant, and place it in clean centrifuge bottles. Discard the pellet.
6. Spin the supernatant at 2100 rpm (~2500xG) for 10 minutes. Discard the supernatant. Resuspend the pellet in about 5 mls of cold thylakoid isolation buffer (without sodium ascorbate). Add what remains of the 200 ml of thylakoid suspension buffer to the suspension.
7. Spin the suspension at 1500 rpm (~1800xG) for one and a half minutes. Collect the supernatant, and place it in clean centrifuge bottles. Discard the pellet.
8. Spin the supernatant at 2100 rpm (~2500xG) for 10 minutes. Discard the supernatant. Resuspend the pellet in about 2 ml of cold thylakoid isolation buffer (without sodium ascorbate).
9. Dilute a 20 µl sample of the final thylakoid suspension in 2 ml of 80% acetone. Filter the solution through Whatman #4 filter paper. Place the filtered solution in a cuvette. Use a cuvette filled with 80% acetone as the blank. Determine the absorbance of the green solution at 663 nm and at 645 nm. The concentration of chlorophyll in the original suspension is calculated from the following equation, where the dilution factor is 100 (2.0 ml/0.020 ml):

$$\text{mg chl/ml} = ((A_{663})(0.00802)+(A_{645})(0.0202)) \text{ x dilution factor.}$$

IworX Sample Lab